



 Sample — fictional facility

CONFIDENTIAL

Sterile processing readiness assessment

Lakeside Surgery Center


Assessed	3 Nov 2025
Assessor	Sample assessor
Report version	v1.0



AN I.M.E. INSTITUTE COMPANY

Sample — fictional facility

Executive summary

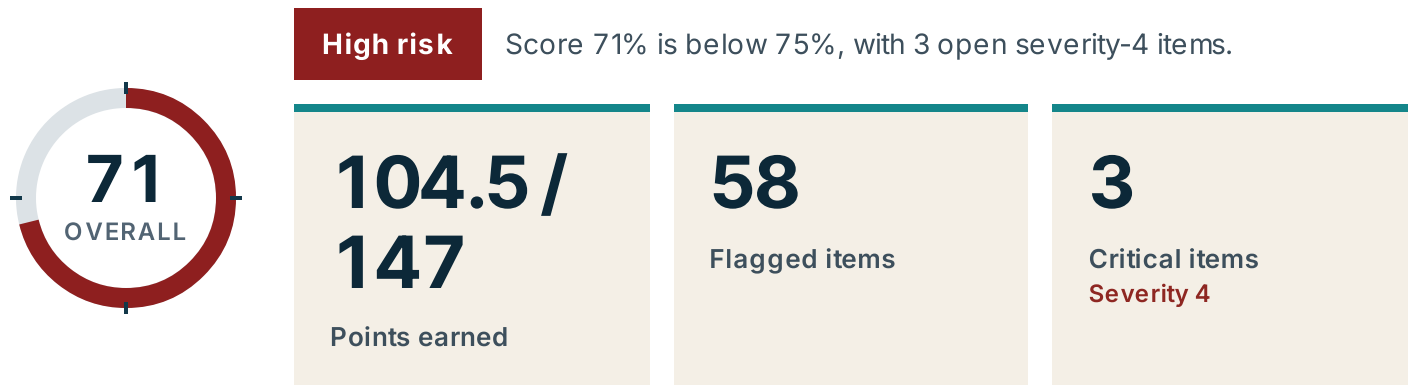


Answer distribution

All questions

147 items




Findings by severity

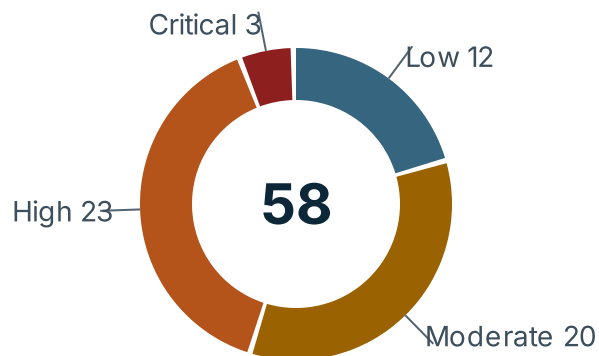

Sample — fictional facility

Section scorecard

Lowest score first. The line marks the 90% survey-ready threshold.

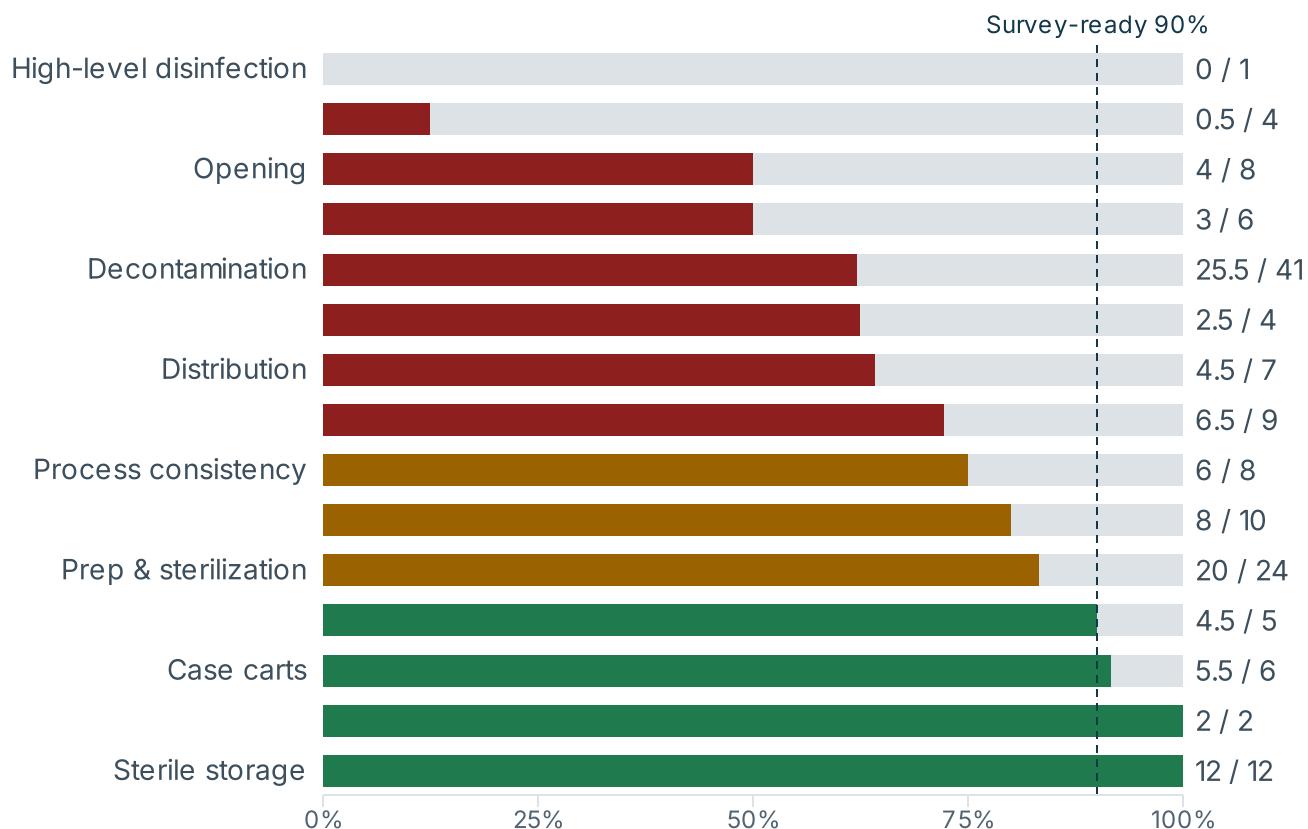

 Sample — fictional facility

Top risks

Each finding names the standard, the gap and the fix.

key DECON-032

 Non-compliant

4 Critical

No eyewash station in decontamination

Install a plumbed or self-contained eyewash within 10 seconds of the sinks before survey.

TJC EC.02.05.01

key DECON-004

 Non-compliant

4 Critical

No hand sink in decontamination

Add a dedicated hand-hygiene sink at the exit from the decontamination room.

TJC IC.02.01.01

key DECON-051

 Non-compliant

4 Critical

Loaner trays skip full decontamination

Route every loaner tray through the full decontamination cycle on receipt.

TJC IC.02.02.01 EP 2